

A circular microscopic image showing numerous thin, needle-like fibers of varying lengths and colors (blue, yellow, orange) against a dark purple background. The fibers are scattered across the field of view, with some appearing in bundles.

California Environmental Protection Agency

 **Air Resources Board**

DRAFT IMPLEMENTATION GUIDANCE DOCUMENT
Good Field Sampling and Laboratory Practices
Test Method 435:
Determination of Asbestos Content of Serpentine Aggregate

Rebecca Domingo-Neumann, Ph.D., P.G.

Jeff Wright, Section Manager

Naturally-Occurring Asbestos Symposium 2014

Association of Environmental & Engineering Geologists (AEG)

December 18, 2014 – Oakland, California

M435 Implementation Guidance Document Topics

- **Introduction**
- **Applicability**
- **Sampling Practices**
- **Sample Processing Practices**
- **Laboratory Sample Analysis**
- **Quality Control**

Introduction

Background

- 1990 ARB Asbestos Airborne Toxic Control Measure (ATCM) for Surfacing Applications.
- 2001 ARB Asbestos ATCM for Construction, Grading, Quarrying, and Surface Mining Operations.
- 2007 ARB M435 Interlaboratory Study (ILS).
 - Sample processing/analytical procedures varied.
 - Can affect reported asbestos content.

Introduction

Purpose


- Assist asbestos stakeholders in the application and performance of M435.
- Clarify procedures and recommend good field sampling and laboratory practices.
- Result in more accurate and repeatable M435 asbestos content measurements.

Applicability of M435

- Surfacing ATCM - M435 is the **required test method** to determine the asbestos content of surfacing aggregate materials.
- Construction ATCM - M435 is referenced as a **laboratory test method** to determine the asbestos content of bulk samples.
- M435 random sampling plan is not applicable for asbestos ATCM exemption requirements.

Sampling Practices for Aggregate Materials


Sources and Sampling Design

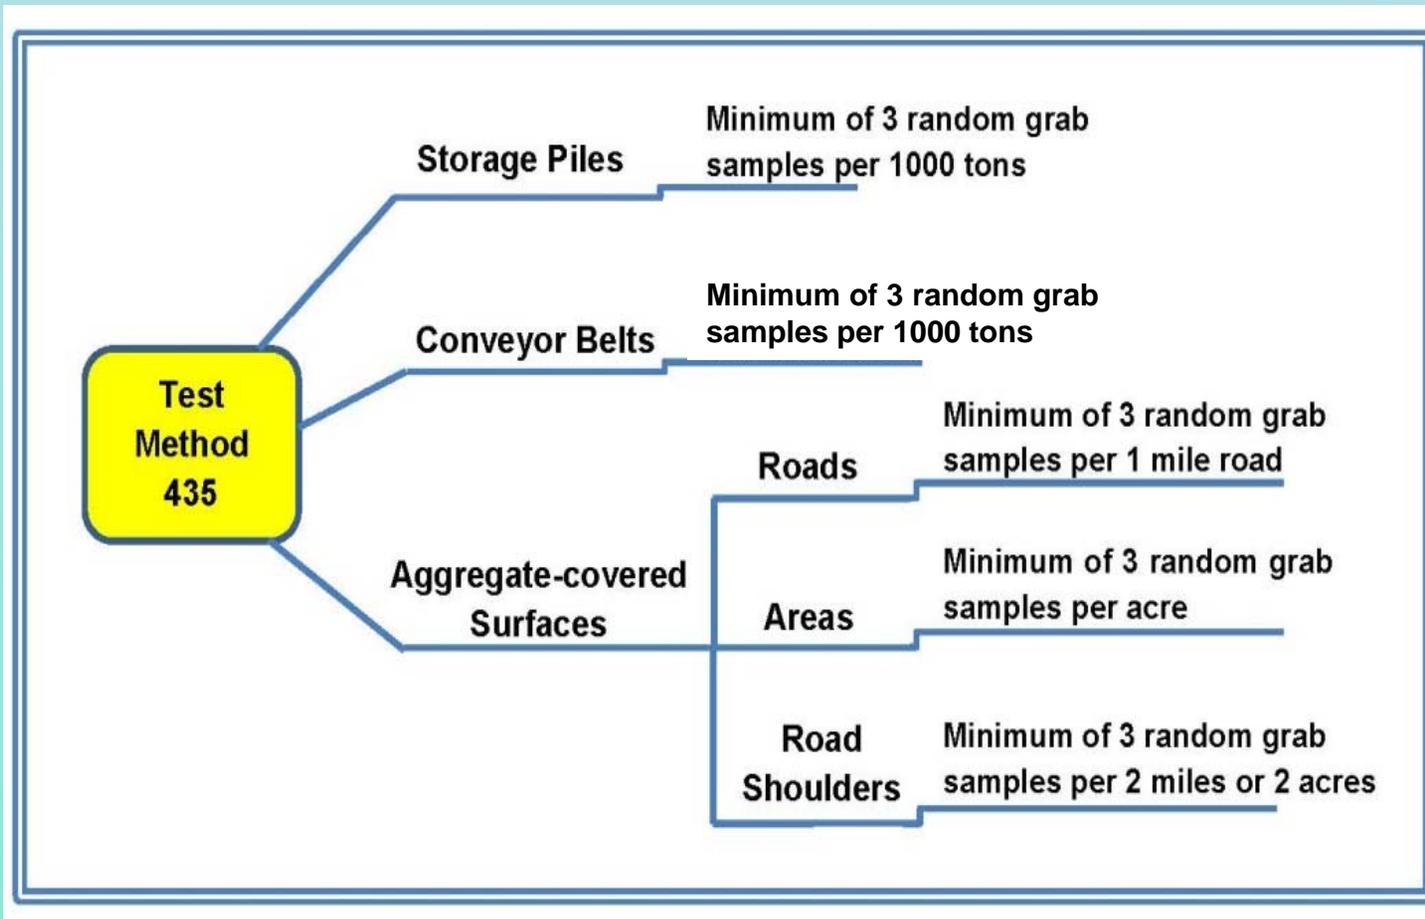

Sampling Practices for Aggregate Materials

Equipment and Procedures

- Storage piles - sloughing effect.
 - Sampling tubes, round point shovels, front loaders.
- Conveyor belts – less sloughing.
 - Automated or manual sampling using templates.
- Aggregate-covered surfaces.
 - Manual or automated augers, shovel, or other suitable equipment.

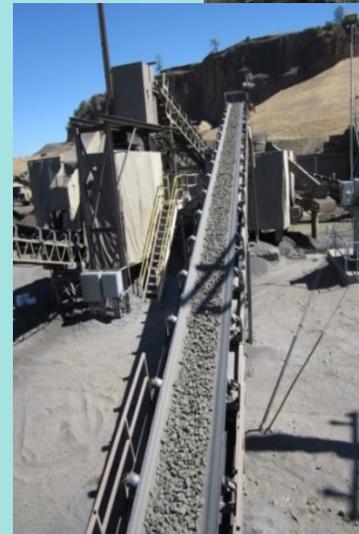

Sampling Practices for Aggregate Materials


Sample Documentation



- Complete sample description per M435.
- Sample acceptance criteria.
- Chain of custody documentation.
- Laboratory information management system.

Laboratory Sample Processing Practices

M435 Sample Processing

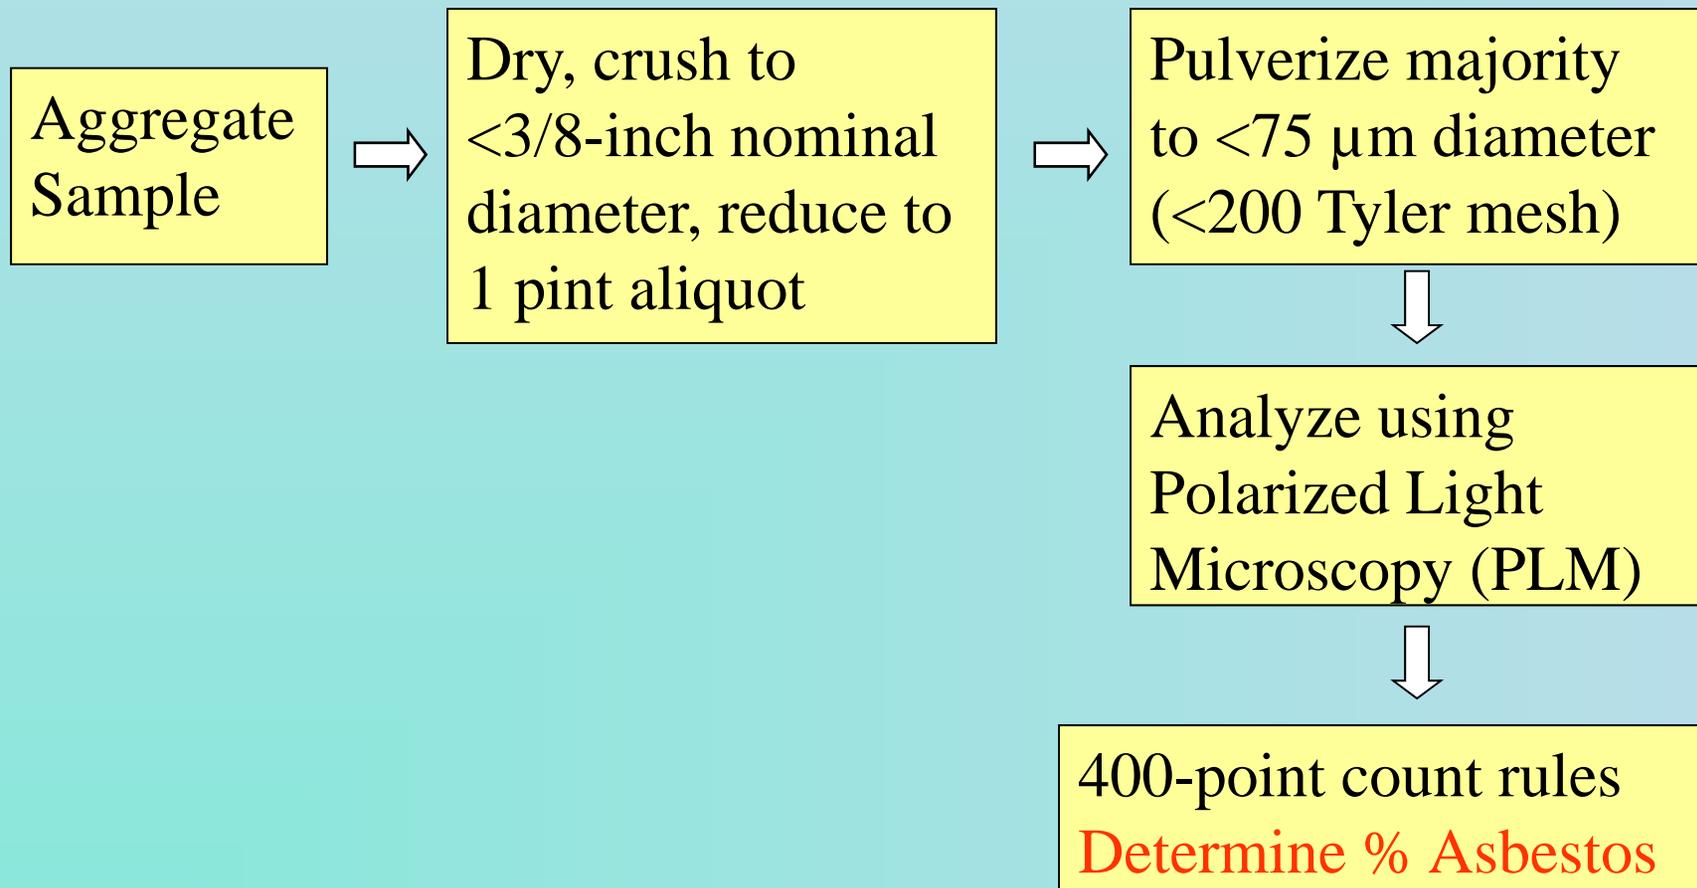

Laboratory Sample Processing Practices

Drying

- Purpose of drying: to remove moisture that would hinder complete pulverization.
- Recommend standardization of laboratory drying procedures (e.g., temperature, time).



Laboratory Sample Processing Practices

Crushing

- Sample must be crushed to a nominal size of $<3/8$ inch (~ 0.95 centimeter).
- Recommend use of jaw crushers:
 - Reliable.
 - Timely.
- Not recommended:
 - Use of hammers.
 - Restricting rock sample sizes.
 - Discarding large rock samples.



Laboratory Sample Processing Practices

Sequence of Post-crushing Procedures

- Post-crushing processing procedures:
 - a) Sample size reduction.
 - b) Homogenization.
 - c) Pulverization.
- The sequence of these procedures affects the representativeness of the powder analyzed.
- The sequence also depends on what equipment are present in the laboratory.

Laboratory Sample Processing Practices

Sequences of Post-crushing Procedures

Available Post-crushing Equipment	Step 1	Step 2	Step 3
Braun Mill + Mixer (Sequence 1)	Pulverize entire crushed sample.	Use mixer to homogenize entire powdered sample.	Manually take 1 pint for analysis.
Braun Mill (no Mixer) (Sequence 2)	Pulverize entire crushed sample.	Manually homogenize powdered sample.	Manually take 1 pint for analysis.
Shatterbox (SB), Ball Mill (BM), or Freezer Mill (FM) + Mixer (Sequence 3)	Use mixer to homogenize entire crushed sample.	Manually take 1 pint crushed sample for pulverization.	Pulverize 1 pint crushed sample for analysis.
SB, BM, or FM (no Mixer) (Sequence 4)	Riffle split entire crushed sample and take 1 pint aliquot.	Pulverize 1 pint crushed sample.	Manually homogenize powdered sample for analysis.
M435: Braun Mill or Equivalent (no Mixer)	Riffle split entire crushed sample and take 1 pint aliquot.	Pulverize 1 pint crushed sample for analysis.	

Test Method 435

Laboratory Sample Processing Practices

Sequences of Post-crushing Procedures

Recommended

Available Post-crushing Equipment	Step 1	Step 2	Step 3
Braun Mill + Mixer (Sequence 1)	Pulverize entire crushed sample.	Use mixer to homogenize entire powdered sample.	Manually take 1 pint for analysis.
Braun Mill (no Mixer) (Sequence 2)	Pulverize entire crushed sample.	Manually homogenize powdered sample.	Manually take 1 pint for analysis.
Shatterbox (SB), Ball Mill (BM), or Freezer Mill (FM) + Mixer (Sequence 3)	Use mixer to homogenize entire crushed sample.	Manually take 1 pint crushed sample for pulverization.	Pulverize 1 pint crushed sample for analysis.
SB, BM, or FM (no Mixer) (Sequence 4)	Riffle split entire crushed sample and take 1 pint aliquot.	Pulverize 1 pint crushed sample.	Manually homogenize powdered sample for analysis.
M435: Braun Mill or Equivalent (no Mixer)	Riffle split entire crushed sample and take 1 pint aliquot.	Pulverize 1 pint crushed sample for analysis.	

Test Method 435

Laboratory Sample Processing Practices

Pulverization

- Recommend the use of the Braun Mill for pulverization.
- ILS results - Braun Mill produced powder with:
 - No leftover chunks.
 - Not over-pulverized.
 - Majority of particles: <math><75\mu\text{m}</math> diameter.



Laboratory Sampling Processing Practices

Pulverization

- Equivalency of other pulverizers to the Braun Mill.
- M435-specific pulverization protocol for this equipment.
- Acceptable particle size distribution (PSD) and equivalent size characteristics.



Laboratory Sample Processing Practices

Pulverization

The recommended PSD:


- $\geq 98\%$ of the powder passes through the 250- μm mesh sieve.
- 75- to 250- μm size fraction is 40 to 50% of the total mass of sample processed.
- $< 75\text{-}\mu\text{m}$ size fraction is 50 to 60% of the initial sample mass.



Laboratory Sample Processing Practices

Homogenization

- Increases powder homogeneity.
- Increases the likelihood that a representative aliquot of the field sample is analyzed.
- Increases accuracy and repeatability.
- Recommend:
 - use of a 3-dimensional mixer.

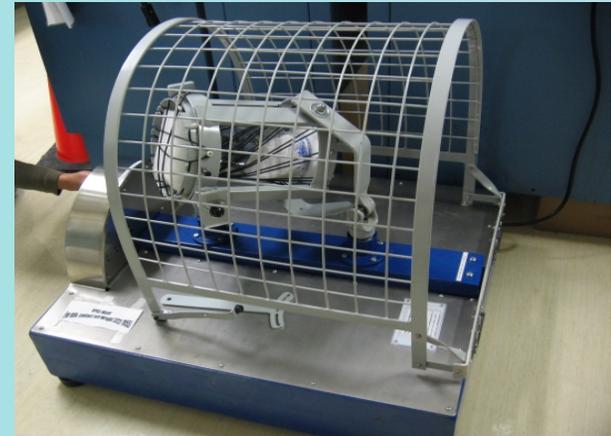

Laboratory Sample Processing Practices

Sample Size Reduction of Crushed Sample


- Even number of equal width chutes.
- At least 8 chutes for coarse aggregate, or 12 chutes for fine aggregate.
- Minimum width of the individual chutes should be about 50% larger than the largest particles in the sample.



Laboratory Sample Analysis Procedures

Principles of M435 Asbestos Identification

- Morphology requirements.
- Optical characteristics determination by polarized light microscopy (M435 Table 3).

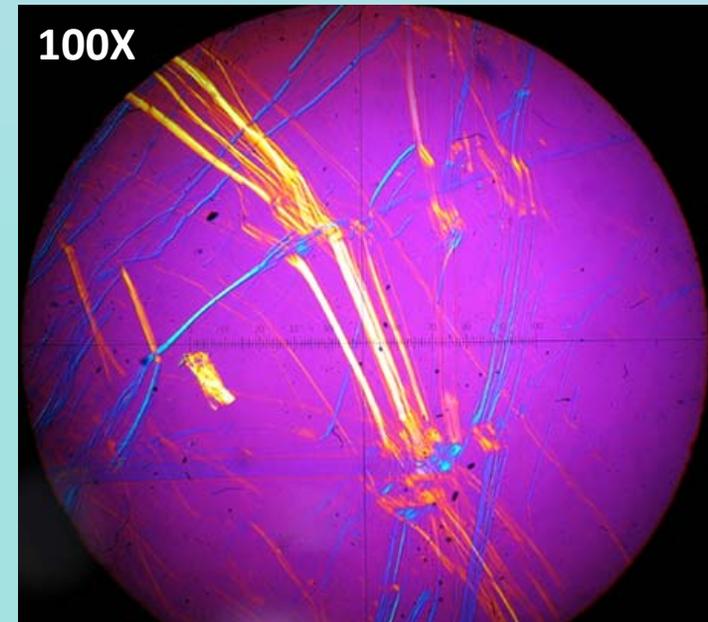

5 mm

Laboratory Sample Analysis Procedures

PLM Resolution

- Fine particles and fibers $\leq 2\mu\text{m}$ in length and $\leq 0.15\mu\text{m}$ in thickness.
- Smaller asbestos fibers may still be present.
- Other analytical techniques are not part of M435:
 - X-ray diffractometry (XRD).
 - Scanning electron microscopy (SEM).
 - Transmission Electron Microscopy (TEM).
- For example, the Department of Toxic Substances Control uses for schools a tiered analytical approach of PLM followed by TEM.

Laboratory Sample Analysis Procedures


Asbestos Quantification

- Required testing volume:
 - 1 pint powdered aliquot.
- Recommended powder mass:
 - 5 mg per PLM slide, particle loading of ~30%.
- Fiber identification requirements:
 - Length-to-width aspect ratio of $\geq 3:1$ **and**
 - Asbestos optical properties (M435 Table 3).
 - Only asbestos characteristics, as described in M435 Table 3, should be used for asbestos identification.

Laboratory Sample Analysis Procedures

Asbestos Quantification

- Recommended point-count reticle:
 - Standard crosshair reticle.
- Additional objective lens recommended:
 - 20X PLM objective to verify optical properties.
- Increase in points counted:
 - Multiples of 400 (e.g., 800, 1,200, 1,600, etc.).
 - Additional points counted may increase false negative errors.

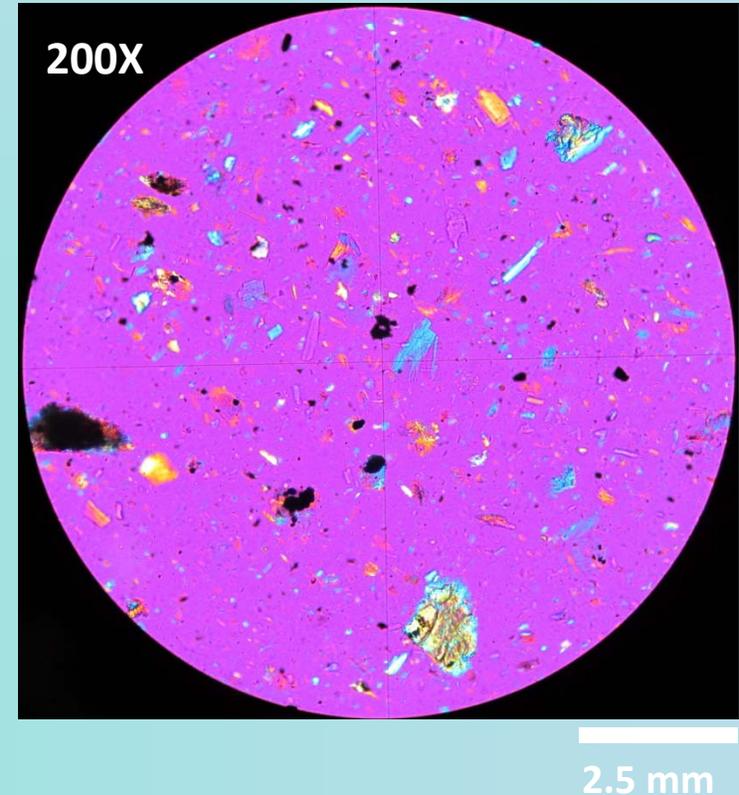

Quality Control Sampling

- Sampling equipment cleanliness.
- Equipment cleaning protocol.
- Integrity of field samples.
- Protection of sample identity.
- Field log of M435 samples, including sampling details.



Quality Control Processing

- Sample chain of custody.
- Laboratory information management system.
- Written SOP specific for M435.
- Processing blanks alongside regular field samples.
- Calibration of processing equipment.
- Particle size calibration check.



Quality Control Analysis

- Microscope alignment.
- Refractive index liquid calibration.
- Asbestos proficiency training.
- Blind analytical replicates.
- Instrument cross checks.
- M435 laboratory protocol validation.
- Performance evaluation slides.
- Documentation of results.



For questions and comments, please contact:

Jeff Wright
Manager, DASPS
jeffrey.wright@arb.ca.gov
916.322.7055

Rebecca D. Neumann, Ph.D., P.G.
Air Pollution Specialist
rebecca.neumann@arb.ca.gov
916.324.1145

Visit the Test Method 435 website and join the Asbestos List Serve:
<http://www.arb.ca.gov/toxics/asbestos/tm435/tm435.htm>

**ARB Monitoring and Laboratory Division
Data Analysis and Special Projects Section (DASPS)
P.O. Box 2815, Sacramento CA 95812**