



California Environmental Protection Agency
Air Resources Board

**Discussion of Potential Changes to
ARB Test Method 435
and Corresponding Amendments to the Asbestos
Airborne Toxic Control Measures**

June 10, 2008 Workshop

Operations Planning & Assessment Section
Quality Management Branch
Monitoring and Laboratory Division

Emissions Evaluations Section
Emissions Assessment Branch
Stationary Source Division

1

Workshop Agenda

- ◆ Introduction
- ◆ Potential Revisions to Method 435 (M435)
- ◆ Corresponding Potential Revisions to Asbestos Airborne Toxic Control Measures (ATCMs)
- ◆ Revision Schedule/Next Workshop

2

Workshop Agenda

- ◆ Introduction
 - Workshop agenda
 - **Revision Schedule**
 - Summary of 1st workshop on 1/24/08
 - Additional topics considered for revision
- ◆ Potential Revisions to Method 435 (M435)
- ◆ Corresponding Potential Revisions to the Asbestos ATCMs
- ◆ Revision Schedule/Next Workshop

3

M435 Revision Schedule

- ◆ January 24, 2008 Workshop (1st)
 - Rationale & identification of areas of M435 examined for revision
- ◆ **June 10, 2008 Workshop(2nd)**
 - **More focused proposed revisions to M435**
 - **Additional topics considered for revision**
- ◆ Fall 2008 Workshop (3rd)
- ◆ 2009 Board Hearing

4

Workshop Agenda

- ◆ Introduction
 - Workshop agenda
 - Revision Schedule
 - **Summary of 1st workshop on 1/24/08**
 - Additional topics considered for revision
- ◆ Potential Revisions to Method 435 (M435)
- ◆ Corresponding Potential Revisions to the Asbestos ATCMs
- ◆ Revision Schedule/Next Workshop

5

Workshop One: M435 Interlaboratory Study Conclusions

- ◆ Laboratories use different sample processing equipment and protocols.
 - Result in varying particle size distribution of processed samples
- ◆ Finer particle size distribution is one factor resulting in lower % asbestos reported.
- ◆ Fiber identification criteria are not uniform among laboratories leading to differences in the % asbestos reported.

6

Topics Discussed in Workshop One

- ◆ Sample Processing
 - Crushing: equipment
 - Pulverization: equipment, particle sizes
- ◆ Sample Analysis
 - Use of reticles, mechanical stage
 - Magnification, point counting
 - Asbestos identification
- ◆ Laboratory Accreditation

7

Workshop Agenda

- ◆ Introduction
 - Workshop agenda
 - Revision Schedule
 - Summary of 1st workshop on 1/24/08
 - **Additional topics considered for revision**
- ◆ Potential Revisions to Method 435 (M435)
- ◆ Corresponding Potential Revisions to the Asbestos ATCMs
- ◆ Revision Schedule/Next Workshop

8

Workshop Two Activities

- ◆ Continue discussion from 1/24/08 Workshop with more focused, proposed revisions
- ◆ Introduce three new topics:
 - Field sampling
 - Addition of transmission electron microscope (TEM) analysis to M435
 - Modifications to ATCMs to reflect changes to M435

9

Workshop Agenda

- ◆ Introduction
- ◆ Summary of 1st Workshop on 1/24/08
- ◆ Potential Revisions to Method 435
 - **Review of ATCMs and M435**
 - Field Sampling
 - Sample Processing
 - Sample Analysis
- ◆ Corresponding Potential Revisions to the Asbestos ATCMs
- ◆ Revision Schedule/Next Workshop ¹⁰

What are the Asbestos ATCMs?

- ◆ Asbestos ATCM for Construction, Grading, Quarrying, and Surface Mining Operations (CCR Section 93105)
 - Requires the implementation of dust mitigation measures where asbestos is known or likely to exist
- ◆ Asbestos ATCM for Surfacing Applications (CCR Section 93106)
 - Restricts the asbestos content of material used in surfacing applications such as unpaved roads, parking lots, driveways, and walkways

11

Asbestos ATCM Applicability

- ◆ Any property that is entirely or partially located in a geographic ultramafic rock unit
- ◆ Any property that is not located in a geographic ultramafic rock unit, but has naturally-occurring asbestos, serpentine, or ultramafic rock
- ◆ Aggregate material that contains at least 10% of materials from ultramafic area or other areas determined to have at least 0.25% asbestos per M435


12

Asbestos ATCM Applicability

- ◆ Surfacing ATCM
 - If testing per M435, applicable at the Limit of Detection = 0.25%
- ◆ Construction ATCM
 - If testing, applicable upon detection of asbestos
- ◆ Intent of both ATCMs
 - Applicable where asbestos is likely to occur (e.g., mapped ultramafic area)
 - Applicable when testing has detected asbestos (e.g., M435)

13

Current Test Method 435 Protocol

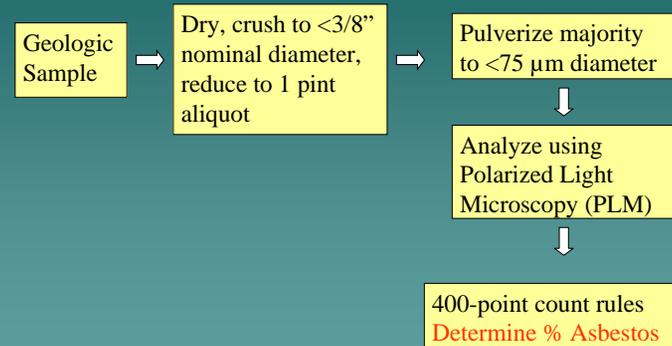

14

Questions?

Workshop Agenda


- ◆ Introduction
- ◆ Summary of 1st Workshop on 1/24/08
- ◆ Potential Revisions to Method 435
 - Review of ATCMs and M435
 - **Field Sampling**
 - Sample Processing
 - Sample Analysis
- ◆ Corresponding Potential Revisions to the Asbestos ATCMs
- ◆ Revision Schedule/Next Workshop 16

Sampling Objective

- ◆ The purpose of geologic sampling is to determine whether asbestos minerals occur at the site under consideration.

17

Current M435 Sampling Method

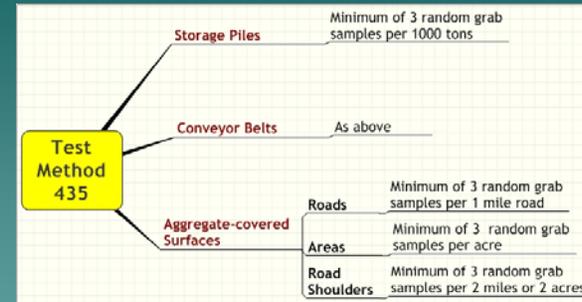

Note: Not specific to Construction ATCM

18

Current Field Sampling Requirements: Who is Qualified?

For areas within ultramafic rock units

- ◆ For the purpose of seeking an exemption: The APCO may provide an exemption . . . if a **registered geologist** has conducted a **geologic evaluation** of the property . . . and determined that no serpentine or ultramafic rock is likely to be found in the area to be disturbed.

-Section 93105 (c)(1) – Construction ATCM

-Section 93106 (f)(7) – Surfacing ATCM

19

Current Field Sampling Requirements: Who is Qualified?

For areas outside ultramafic rock units:

- ◆ “However, the ATCM does allow the districts to request a **geologic evaluation** on property outside of a geographic ultramafic rock unit.”

-Section VII.A.1. Guidance Document for Surfacing ATCM

20

Proposed Field Sampling Requirements: Who is Qualified?

For areas outside ultramafic rock units:

- ◆ The geologic evaluation of a site requires a registered geologist

21

Current Sampling Strategy

- ◆ Random sampling
 - 3 “grab samples” composited into one laboratory sample

22

Proposed Field Sampling Strategies

Requires an initial geologic assessment to decide which strategy is appropriate:

- ◆ **Targeted Sampling**
 - Appropriate when asbestos is more likely to be present at one location than at another due to its geologic occurrence
- ◆ **Random Sampling**
 - Appropriate when sampling personnel has concluded that asbestos is no more likely to occur in one area than another

23

Current Field Sampling: Sample Number & Volume

- ◆ 3 grab samples = 1 composited sample
 - per acre of area, or mile of road, or 1000 tons of aggregate
- ◆ 3 grab samples = 1 composited sample
 - per 2 acres or 2 miles of aggregate-covered road shoulder
- ◆ Minimum volume of composited sample = 1 pint
 - Composited samples are analyzed following M435

24

Proposed Field Sampling Strategies: Sample Number and Volume

Current	Proposed
Minimum of three field samples per acre/1000 tons/mile	Same
Composited	Composited (random) Separate (targeted) -to test specific features, e.g., veins or fracture fillings
Minimum composited sample volume = 1 pint	Minimum field sample volume = 0.5 liter (~1.1 pint) Minimum composited sample volume = 1.5 L (~3.3 pints) 25

Current Field Sampling: Depth of Samples

- ◆ Sample depth is currently not addressed by M435 sampling protocol

26

Proposed Field Sampling Strategies: Depth of Samples


- ◆ Surface to depth expected to be disturbed
- ◆ Separate samples when distinct changes in soil horizons (e.g., A, B, Cr) or lithology are observed

27

Workshop Agenda

- ◆ Introduction
- ◆ Summary of 1st Workshop on 1/24/08
- ◆ Potential Revisions to Method 435
 - Review of ATCMs and M435
 - Field Sampling
 - **Sample Processing**
 - Sample Analysis
- ◆ Corresponding Potential Revisions to the Asbestos ATCMs
- ◆ Revision Schedule/Next Workshop 28

Current Test Method 435 Protocol

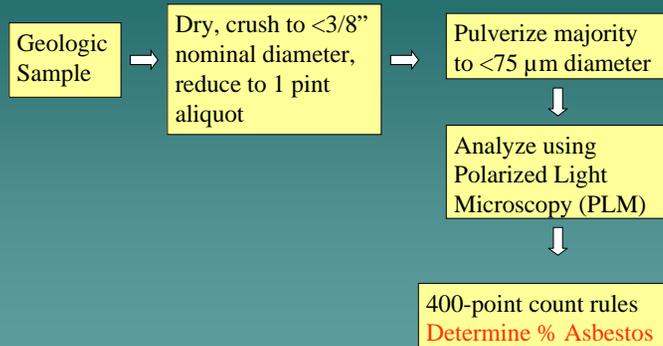

29

Sample Processing: Key Elements of Proposed Protocol

Currently written in M435:


- ◆ Use of Braun mill (plate grinder)
 - allows calibration of pulverization process
 - can process larger volume more quickly
- ◆ Entire field sample processed

Proposed processing for M435 samples:

- ◆ Pre-sieving procedure to remove fine fractions early in the process
 - avoids over-pulverization of material

30

Summary: Proposed Sample Processing

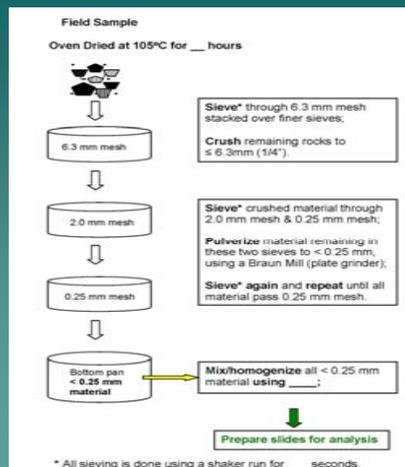

31


Proposed Sample Processing: Standardize Drying Procedure

- ◆ Drying of samples at 105 C
- ◆ Drying time to be determined depending on sample volume



32

Proposed Sample Processing: Pre-sieving of Field Sample

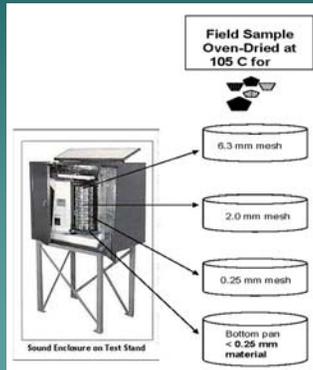

- ◆ Pour field sample into 6.3 mm sieve stacked over finer sieves (i.e., 2 mm, 0.25 mm) and bottom pan.
- ◆ Run shaker for ____ minutes.
- ◆ All sieving must be done using a shaker.

33


Proposed Sample Processing: Pre-sieving of Field Sample

- ◆ Separates fine particles that do not need further pulverization



Proposed Sample Processing: Crushing of Coarse Fraction

- ◆ Crush material remaining on 6.3 mm sieve to <6.3 mm (1/4 inch) using a Jaw rock crusher
- ◆ Sieve material through 2 mm & 0.25 mm mesh

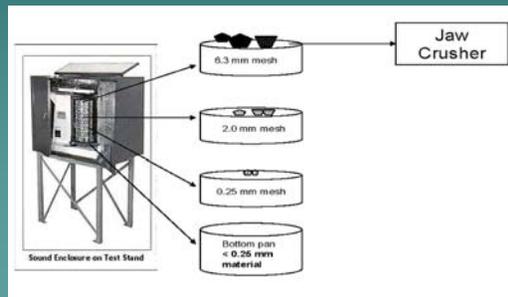

35

Proposed Sample Processing: Crushing of Coarse Fraction


- ◆ Crushing of large samples to 6.3 mm (1/4") nominal size
 - Needed to reduce size of rock for use in Braun Mill pulverizer
 - Use Jaw rock crusher



36

Proposed Sample Processing: Pulverization of Field Sample

- ◆ Pulverize material remaining on 2 mm & 0.25 mm sieves to <0.25 mm using a Braun Mill
- ◆ Repeat pulverization and sieving until all material pass through 0.25 mm sieve

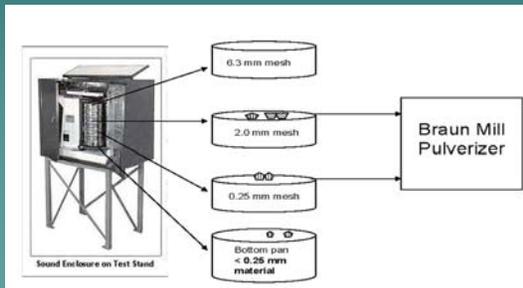

37

Proposed Sample Processing: Sample Pulverization

- ◆ Calibrate so that majority of powder is >75 um and 100% <250 um




Braun Mill (Plate Grinder)

38

Proposed Sample Processing: Homogenization of Pulverized Sample

- ◆ Mix/homogenize <0.25 mm material
- ◆ Use for slide preparations

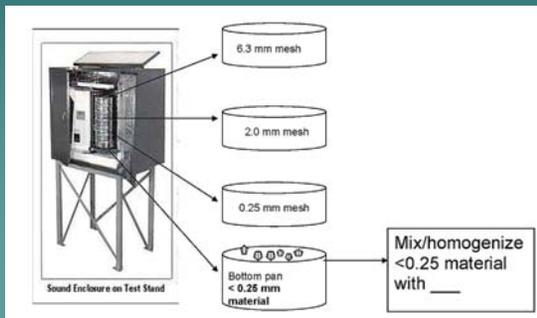

39

Workshop Agenda

- ◆ Introduction
- ◆ Summary of 1st Workshop on 1/24/08
- ◆ Potential Revisions to Method 435
 - Field Sampling
 - Sample Processing
 - **Sample Analysis**
- ◆ Corresponding Potential Revisions to the Asbestos ATCMs
- ◆ Revision Schedule/Next Workshop

40

Proposed Analysis Objective

- ◆ Asbestos detection will be the object of sample analysis.


41

Proposed Stereoscopic Scan, PLM, and TEM Analyses

- ◆ Stereoscopic scan of unprocessed samples
 - Suspect fibers analyzed by PLM
- ◆ PLM analysis of processed samples
 - Evaluates a larger sample mass than TEM
- ◆ TEM analysis when asbestos is not detected by PLM
 - Higher magnification than PLM; smaller sample mass
 - Energy-dispersive spectra for elemental composition of particles
 - Diffraction patterns for mineralogy


42

Proposed Analysis Flowchart

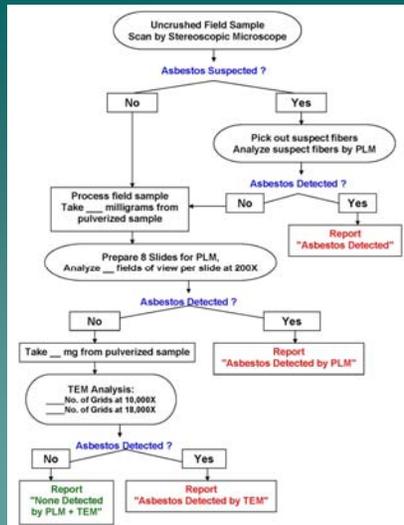

43

Proposed Analysis Flowchart: Low Mag. Sample Scan

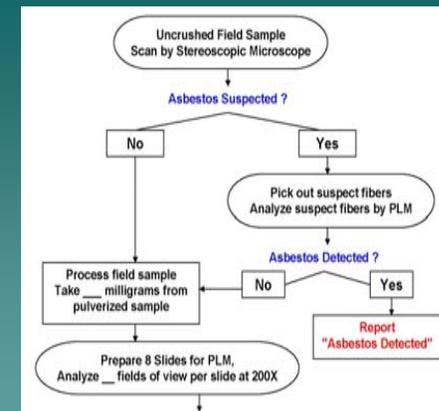

44

Proposed Analysis: Low Magnification Stereoscope


- ◆ Observe unprocessed sample with a stereoscopic microscope to look for suspect fibers
- ◆ Prepare oil immersion slides of suspect fibers and analyze by PLM
- ◆ Report if asbestos detected



45

Proposed Analysis Flowchart:

PLM and TEM Analyses

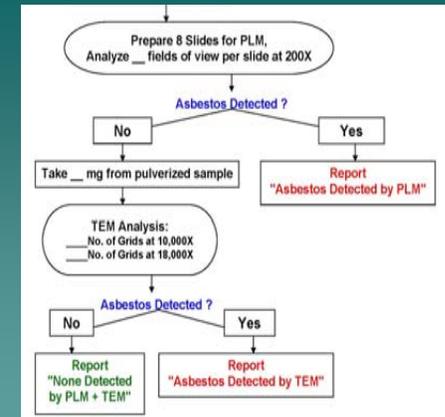

46

Proposed Analysis: Asbestos Detection by PLM

- ◆ Process entire field sample
- ◆ Weigh ? milligrams of powdered sample
- ◆ Prepare 8 slides for PLM analysis
- ◆ All of the weighed out material must be prepared on the slides
- ◆ Scan entire slides at 200X using ? number of non-overlapping fields of view evenly distributed throughout the slide
- ◆ Report if asbestos is detected

47

Proposed Analysis: Magnification & Mechanical Stage

- ◆ Magnification of 200X for asbestos identification
- ◆ Use of mechanical stage and point counting knobs for evenly spaced fields of view on entire slide



48

Proposed Analysis: Asbestos Detection by TEM

- ◆ Major issues to be resolved:
 - Sample preparation
 - Amount of material for TEM preparations
 - Analytical conditions: magnifications, number of grid openings analyzed
 - Use of energy-dispersive X-ray analysis
 - Use of selected area diffraction patterns and Kikuchi patterns
 - Calculation of asbestos concentrations

49

Suggest New References for Optical Analysis of Asbestos

- ◆ What references should laboratories use for identification of asbestos by PLM?
 - For proposed Table 3 - optical properties of asbestos fibers
 - For proposed Table 4 – central stop staining dispersion colors

50

Suggest New References for TEM Analysis

- ◆ What references should laboratories use for identification of asbestos by TEM?
 - For proposed Table 5 - asbestos characteristics observed with TEM
 - References for energy-dispersive X-ray spectra
 - References for diffraction patterns

51

Questions?

Workshop Agenda

- ◆ Introduction
- ◆ Potential Revisions to Method 435
- ◆ **Corresponding Potential Revisions to the Asbestos ATCMs**
 - Asbestos definition
 - Laboratory accreditation
 - Detection levels
- ◆ Revision Schedule/Next Workshop

53

Workshop Agenda

- ◆ Introduction
- ◆ Potential Revisions to Method 435
- ◆ Corresponding Potential Revisions to the Asbestos ATCMs
 - **Asbestos definition**
 - Laboratory accreditation
 - Detection levels
- ◆ Revision Schedule/Next Workshop

54

Asbestos Definition

- ◆ Clarify asbestos definition in the ATCMs
 - Define terms used in asbestos definition
 - Reference optical and chemical properties in M435
- ◆ Maintain consistency with the formal identification of asbestos as a Toxic Air Contaminant (TAC)

55

Current Asbestos Definition

- ◆ Asbestos - "asbestiform varieties of the following minerals: chrysotile (fibrous serpentine), crocidolite (fibrous riebeckite), amosite (fibrous cummingtonite—grunerite), fibrous tremolite, fibrous actinolite, and fibrous anthophyllite."
 - Surfacing ATCM and Construction ATCM

56

Proposed Asbestos Definition

- ◆ Clarify asbestos definition by defining “asbestiform”
 - Consistent with health effects known at time of formal identification as TAC
 - Consistent with health effects known today

57

Proposed Asbestiform Definition

- ◆ Asbestiform – A term to describe a mineral determined to have:
 - Optical properties within specified range if using PLM
 - Chemical properties within specified range if using TEM
 - Fiber aspect ratio of 3:1 or greater
 - Width less than 3 μm (individual fiber)
 - No length criteria

58

Proposed Asbestiform Definition

- ◆ Asbestiform (asbestos) is any of “the six” minerals having various morphological and physical features including, but not limited to:
 - Acicular or needle-like crystal habit
 - Cleavage planes bounding fragments
 - Irregular shapes
 - ◆ Square terminations
 - ◆ Non-parallel or jagged sides

59

Workshop Agenda

- ◆ Introduction
- ◆ Potential Revisions to Method 435
- ◆ Corresponding Potential Revisions to the Asbestos ATCMs
 - Asbestos definition
 - **Laboratory accreditation**
 - Detection levels
- ◆ Revision Schedule/Next Workshop

60

Proposed ATCM Requirement: M435 Accreditation

- ◆ Add a provision that requires “M435 laboratory accreditation” when testing is done per M435

61

Proposed M435 Laboratory Accreditation

- ◆ NVLAP - National Voluntary Laboratory Accreditation Program
- ◆ NELAP/ELAP - National Environmental Laboratory Accreditation Program / California ELAP within the California Department of Public Health

62

Workshop Agenda

- ◆ Introduction
- ◆ Potential Revisions to Method 435
- ◆ Corresponding Potential Revisions to the Asbestos ATCMs
 - Asbestos definition
 - Laboratory accreditation
 - **Detection levels**
- ◆ Revision Schedule/Next Workshop

63

Restricted Material

- ◆ Current - set at 0.25% or greater asbestos content
- ◆ Proposed - will reflect the detection of asbestos as determined by M435

64

Questions?

Workshop Agenda

- ◆ Introduction
- ◆ Potential Revisions to Method 435
- ◆ Corresponding Potential Revisions to the Asbestos ATCMs
 - Asbestos definition
 - Laboratory accreditation
 - Detection levels
- ◆ **Revision Schedule/Next Workshop**

66

M435 Revision Schedule

- ◆ January 24, 2008, Workshop (1st)
- ◆ June 10, 2008 Workshop (2nd)
 - Comments on proposed revisions to M435 and ATCMs
- ◆ **Fall 2008 Workshop (3rd)**
- ◆ 2009 Board Hearing

67

Workshop Three

- ◆ Time frame: Fall 2008
- ◆ Time of day: ?
- ◆ Possible venue: ?

68



California Environmental Protection Agency
Air Resources Board

June 10, 2008 Workshop

*Thank you for your participation.
For questions and comments, please contact:*

Jeff Wright
Manager
Operations Planning & Assessment
jwright@arb.ca.gov
916.322.7055

Rebecca D. Neumann
Air Pollution Specialist
OPAS
rneumann@arb.ca.gov
916.324.1145

Air Resources Board
P.O. Box 2815, Sacramento CA 95812

69